
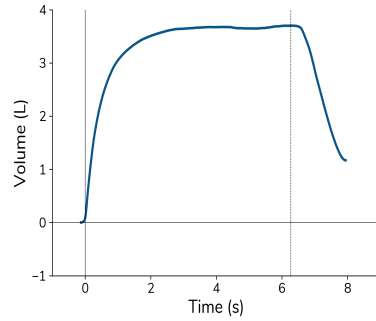


TRIAL 2

FEV1 **Acceptable**

FVC **Usable** (failure of EOT criteria)

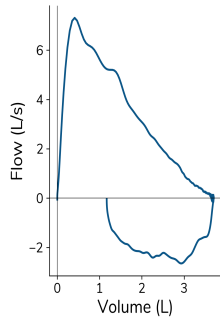

BEV Criteria: **True**
 EO) Criteria: **False**
 Plateau Criteria: **False**
 (52.98 mL change in last second)
 tFE > 15s: **False**
 FIVC-FVC Criteria: **None**

No artefact on MEFVC


Warnings

Insufficient second inspiration

TRIAL 3

FEV1 **Acceptable**

FVC **Acceptable**

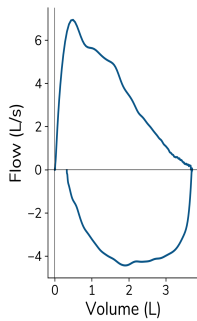

BEV Criteria: **True**
 EO) Criteria: **True**
 Plateau Criteria: **True**
 (16.75 mL change in last second)
 tFE > 15s: **False**
 FIVC-FVC Criteria: **True**

No artefact on MEFVC

Warnings

Leak/neg flow error

TRIAL 4

FEV1 **not Acceptable or Usable** (Artefact (P=0.68) on MEFVC<1s (Hesitation))

FVC **Acceptable**

BEV Criteria: **True**
 EO) Criteria: **True**
 Plateau Criteria: **False**
 (45.02 mL change in last second)
 tFE > 15s: **False**
 FIVC-FVC Criteria: **True**

Artefact on MEFVC<1s (Hesitation)



Warnings

Rise time

TRIAL 5

FEV1 **Acceptable**

FVC **Acceptable**

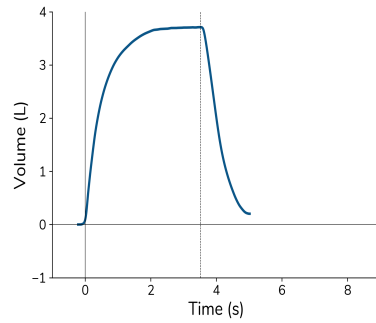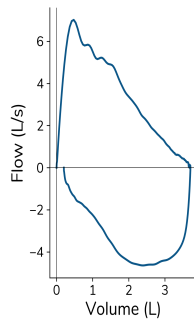

BEV Criteria: **True**
EOFE Criteria: **True**
Plateau Criteria: **False**
(28.12 mL change in last second)
tFE > 15s: **False**
FIVC-FVC Criteria: **True**

No artefact on MEFVC

Warnings

None